

S. JOHN MARY¹,
SUSAI RAJENDRAN²

Scientific paper
UDC:620.193.4:612.397

Corrosion behavior of Cu-Ni-Ti in artificial blood plasma in presence of cholesterol

The Corrosion behaviour of Cu-Ni-Ti in artificial blood plasma in absence and presence of 50ppm and 100ppm of Cholesterol were studied by potentiodynamic polarization study and AC impedance spectra. The inhibition efficiencies of Cholesterol for the corrosion of Cu-Ni-Ti is increased with increasing concentration. Potentiodynamic polarization study shows that the corrosion of metal surface is greatly reduced with presence of Cholesterol. This may occur due to the formation of protective layer formed on the metal in presence of Cholesterol. The polarization study leads to the corrosion inhibition of Cu-Ni-Ti in artificial blood plasma in absence and presence of 50 ppm of Cholesterol and 100 ppm of cholesterol is in the following decreasing order:

Cu-Ni-Ti + artificial blood plasma + 100 ppm of Cholesterol > Cu-Ni-Ti + artificial blood plasma + 50 ppm of Cholesterol > Cu-Ni-Ti + artificial blood plasma

The AC impedance spectra study reveals that the corrosion inhibition of Cu-Ni-Ti in artificial blood plasma in absence and presence of 50 ppm of Cholesterol and 100 ppm of Cholesterol is in the following decreasing order:

Cu-Ni-Ti + artificial blood plasma + 100 ppm of Cholesterol > Cu-Ni-Ti + artificial blood plasma + 50 ppm of Cholesterol > Cu-Ni-Ti + artificial blood plasma

Keywords: Corrosion, artificial blood plasma, Cu-Ni-Ti, Cholesterol

INTRODUCTION

Cu-Ni-Ti is the most commercially successful implantation material in biomedical [1]. Cu-Ni-Ti alloys are important materials for biomedical and dental devices because of their unique properties, comparatively high corrosion resistance and good biocompatibility. The alloy has been used for making orthodontic dental arch wires and medical guide wires for diagnostic and therapeutic catheters for many years. Corrosion reduces strength and causes premature failure of implants and may also impose harmful effects on the surrounding tissues. Stainless steels, titanium alloys and cobalt alloys are commonly used as biomaterials [2]. Cholesterol is a waxy, fat-like substance that occurs naturally in all parts of the body. Our body needs some cholesterol to work properly. But if we have too much in our blood, it can stick to the walls of our arteries. Cholesterol is present in higher concentrations in tissues which either produce more or have more densely-packed membranes. Cholesterol plays a central role in many biochemical processes, but is best known for the association of cardiovascular disease with various lipoprotein cholesterol transport patterns and high levels of cholesterol in the blood.


Author's address: ¹Dept. of Chemistry, Loyola College, Chennai, India - 600 034, ²Corrosion Research centre, P.G. & Research Dept. of Chemistry, G.T.N. Arts College, Dindigul, Tamilnadu, India-624005

Received for Publication: 13. 03. 2014.

Accepted for Publication: 29. 05. 2014.

Cholesterol is required to build and maintain cell membranes; it makes the membrane's fluidity - degree of viscosity - stable over wider temperature intervals. Some research indicates that cholesterol may act as an antioxidant. Cholesterol also aids in the manufacture of bile (which helps digest fats), and is also important for the metabolism of fat-soluble vitamins, including vitamins A, D, E and K. It is the major precursor for the synthesis of vitamin D and of the various steroid hormones. People who have undergone implantation with high level cholesterol are recommended by medical practitioners to take proper nutritional food to reduce the cholesterol. By eating balanced nutritional food leads to increase or decrease of cholesterol level in our body. The present study reveals whether the implantation materials are affected or corroded due to the intake of cholesterol containing nutritional food.

Structure of Cholesterol

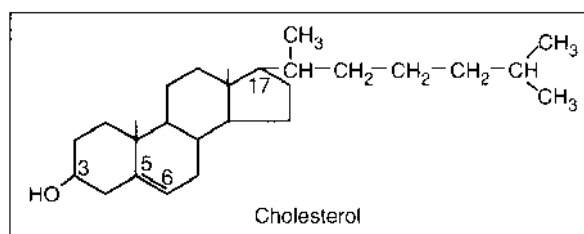

MATERIALS AND METHODS

The metal specimens, namely, Cu-Ni-Ti has been chosen for the present study. The composition focus Cu-Ni-Ti is Ni- 55.5%, Ti -37%, Cu- 7.50% balance [2]. The metal specimen was

encapsulated in Teflon. The metal specimen was polished to mirror finish and degreased with trichloroethylene. The metal specimen was immersed in artificial plasma. The pH of artificial blood plasma was 7.0. The chemical composition of the artificial plasma according to PN-EN ISO 10993-15 standard (g/l distilled water) was NaCl 6.8, CaCl₂ 0.200, KCl 0.4, MgSO₄ 0.1, NaHCO₃ 2.2, Na₂HPO₄ 0.126, NaH₂PO₄ 0.026[3]. In electrochemical studies the metal specimen was used as working electrode plasma was used as electrolyte (10 ml). The temperature was maintained at 37°C.

Potentiodynamic Polarization

Polarization studies were carried out in a CHI – Electrochemical workstation with impedance, Model 660A. A three-electrode cell assembly was used. The working electrode was Cu-Ni-Ti alloy. A saturated calomel electrode (SCE) was the reference electrode and platinum was the counter electrode. From the polarization study, corrosion parameters such as corrosion potential (E_{corr}), corrosion

current (I_{corr}) and Tafel slopes (anodic = b_a and cathodic = b_c) were calculated.

AC Impedance Spectra

The instrument used for polarization study was used to record AC impedance spectra also. The cell setup was also the same. The real part (Z') and imaginary part (Z'') of the cell impedance were measured in ohms at various frequencies. Values of the charge transfer resistance (R_t) and the double layer capacitance (C_{dl}) were calculated from Nyquist plots, impedance $\log(Z/\text{ohm})$ value was calculated from bode plots.

RESULTS AND DISCUSSIONS

Analysis of Potentiodynamic Polarization curves

The corrosion parameters of Cu-Ni-Ti in artificial blood plasma (ABP) are given in Table 1. The potentiodynamic polarization curves are shown in Figs. 1 to 3.

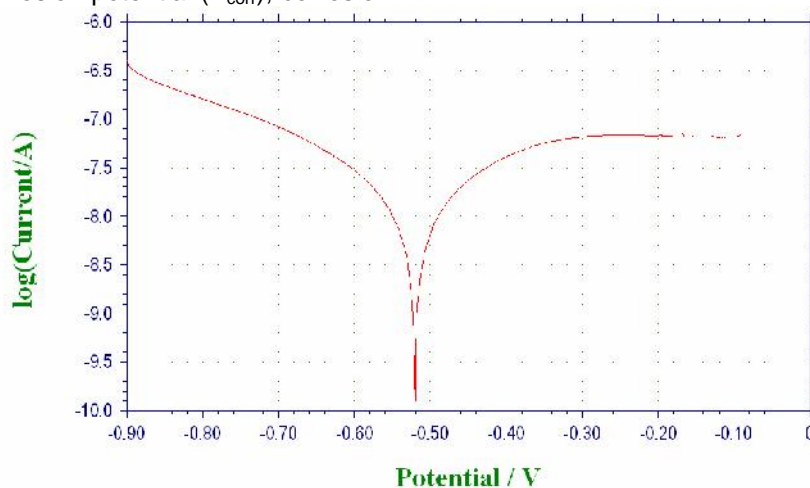


Figure 1 - Polarization curves of Cu-Ni-Ti immersed in artificial blood plasma in absence of Cholesterol.

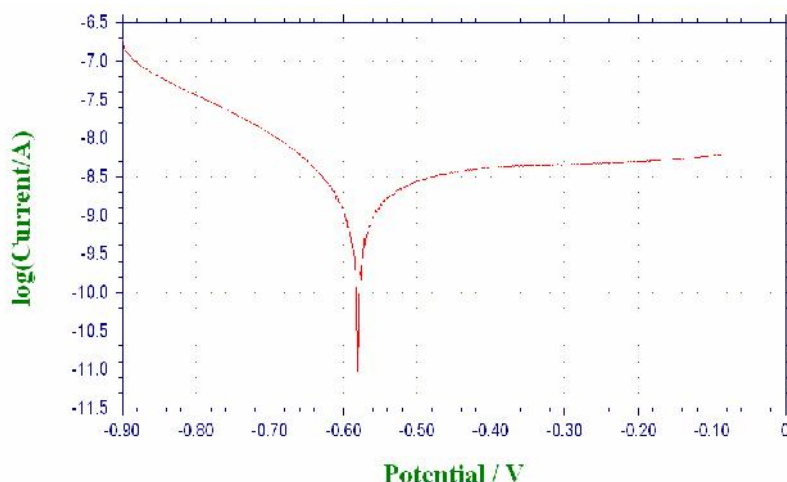


Figure 2 - Polarization curves of Cu-Ni-Ti immersed in artificial blood plasma in presence of 50 ppm Cholesterol.

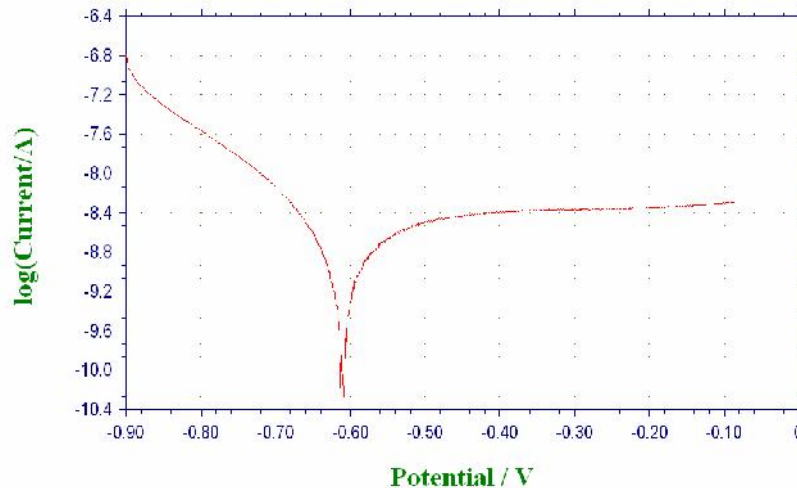


Figure 3 - Polarization curves of Cu-Ni-Ti immersed in artificial blood plasma in presence of 100 ppm Cholesterol.

Cu-Ni-Ti immersed in Cholesterol

The Potentiodynamic polarization curves of Cu-Ni-Ti immersed in artificial plasma in absence and presence of 50ppm Cholesterol and 100 ppm Cho-

lesterol are shown in fig 1, 2 and 3. The corrosion parameters namely corrosion potential, corrosion current (I_{corr}), Tafel slopes b_a , b_c , (LPR) linear polarization resistance are given in the Table 1.

Table 1 - Corrosion parameters of Cu-Ni-Ti immersed in artificial blood plasma in the absence and presence of Cholesterol obtained by polarization study

System	E_{Corr} mV vs SCE	b_c mV/decade	b_a mV/decade	LPR ohm cm^2	I_{Corr} A/ cm^2
Cu-Ni-Ti +ABP	-520	173	195	3.0×10^6	1.329×10^{-8}
-Ni – Ti +ABP +50ppm Cholesterol	-580	137	324	9.88×10^6	2.109×10^{-9}
Cu-Ni – Ti +ABP +100ppm Cholesterol	-609	148	348	2.0×10^7	2.104×10^{-9}

Cu-Ni-Ti immersed in artificial plasma in the absence of Cholesterol

When Cu-Ni-Ti immersed in artificial plasma, the corrosion potential is -520mV Vs SCE. The LPR value is 3.0×10^6 ohm cm^2 and the corrosion current (I_{corr}) is 1.329×10^{-8} A/ cm^2 . The Tafel slope values $b_c = 173$ mV/decade $b_a = 195$ mV/decade indicate that the rate of change of corrosion current with potential is much higher during the cathodic polarization than during the anodic polarization.

Corrosion behavior of Cu-Ni-Ti in artificial blood plasma in presence of 50 ppm of Cholesterol

When Cu-Ni-Ti immersed in ABP in presence of 50 ppm of Cholesterol the corrosion potential is shifted from -520 to -580 mV Vs SCE. The Tafel slopes are $b_c = 137$ mV/decade and $b_a = 324$ mV/decade. The LPR value increases from 3.0×10^6 ohms cm^2 to 9.88×10^6 ohm cm^2 . The corrosion

current (I_{corr}) decreases from 1.329×10^{-8} A/ cm^2 to 2.109×10^{-9} A/ cm^2 . Thus polarization study confirms the formation of a protective film on the metal surface. The polarization study reveals that the corrosion resistance of Cu-Ni-Ti in ABP increases in presence of 50 ppm of Cholesterol.

Corrosion behavior of Cu-Ni-Ti in artificial blood plasma in presence of 100 ppm of Cholesterol

When Cu-Ni-Ti is immersed in artificial blood plasma in presence of 100 ppm of Cholesterol the corrosion potential is shifted from -520 to -609mV Vs SCE. The Tafel slopes are $b_c = 148$ mV/decade and $b_a = 348$ mV/decade. The LPR value increases from 3.0×10^6 to 2.0×10^7 ohm cm^2 . The corrosion current (I_{corr}) decreases from 1.329×10^{-8} to 2.104×10^{-9} A/ cm^2 . Thus the polarization study confirms the formation of a protective film on the metal surface.

The polarization study reveals that the corrosion resistance of Cu-Ni-Ti in ABP in presence of 100 ppm increases. The corrosion resistance of

Cu-Ni-Ti in artificial blood plasma is in the following decreasing order:

$$\text{Cu-Ni-Ti + plasma +100 ppm Cholesterol} > \text{Cu-Ni-Ti + plasma+ 50 ppm Cholesterol} > \text{Cu-Ni-Ti +plasma}$$

AC impedance spectra

The instrument used for polarization study was used to record AC impedance spectra also. The cell setup was also the same. The real part (Z') and imaginary part (Z'') of the cell impedance were measured in ohms at various frequencies. The Values of the charge transfer resistance (R_t) and the double layer capacitance (C_{dl}) were calculated.

Table 2 - Corrosion parameters of Cu-Ni- Ti immersed in artificial blood plasma in the absence and presence of Cholesterol obtained by AC Impedance spectra.

Metal	System	Nyquist plot		Bode plot
		R_t ohm cm^2	C_{dl} F/ cm^2	Impedance log (z/ohm)
Cu-Ni-Ti	Cu-Ni-Ti +ABP	4588	1.11×10^{-11}	5.5
Cu-Ni-Ti	Cu-Ni-Ti +ABP +50ppm Cholestrol	50094	1.0×10^{-10}	4.9
Cu-Ni-Ti	Cu-Ni-Ti +ABP +100ppm cholesterol	52260	9.7×10^{-11}	4.9

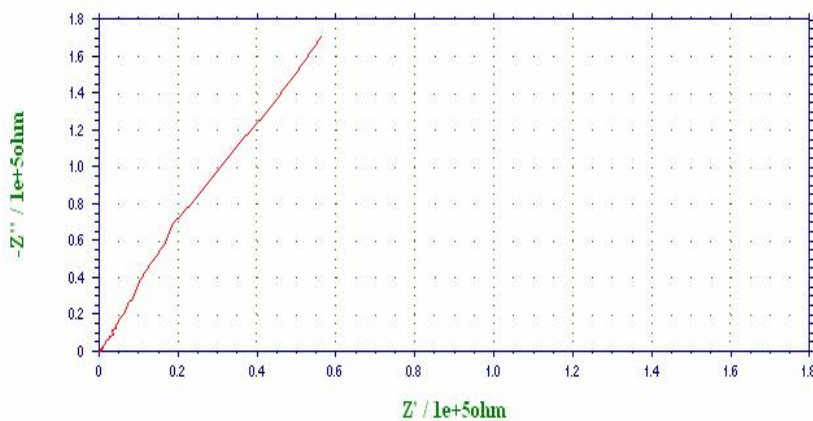


Figure 4 - AC impedance spectra of Cu-Ni-Ti immersed in ABP in absence of Cholesterol (Nyquist Plot).

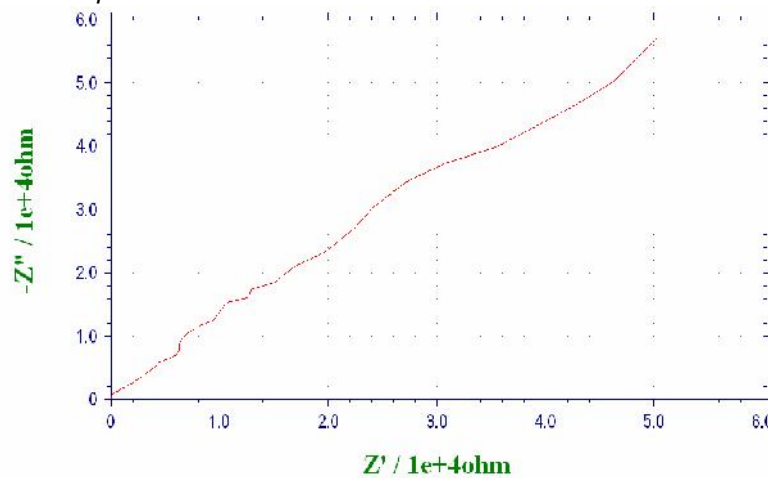


Figure 5 - AC impedance spectra of Cu-Ni-Ti immersed in ABP in presence of 50 ppm Cholesterol (Nyquist Plot).

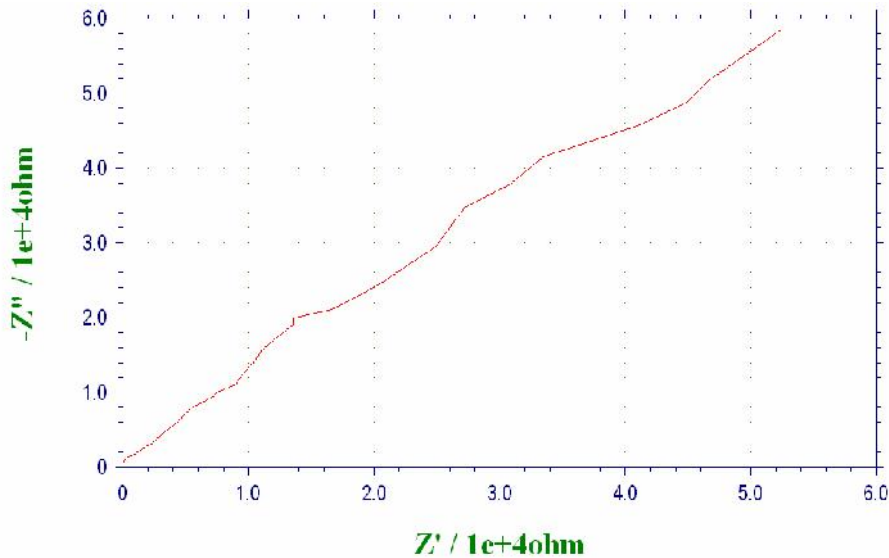


Figure 6 - AC impedance spectra of Cu-Ni –Ti immersed in ABP in presence of 100 ppm Cholesterol (Nyquist Plot).

Cu-Ni-Ti immersed in ABP in absence of Cholesterol

When Cu-Ni-Ti immersed in ABP, the charge transfer resistance R_t is 4588 ohmcm^2 . The double layer capacitance value is $1.11 \times 10^{-11} \text{ F/cm}^2$ Fig. 4. The impedance value is 5.5 Fig. 7.

Cu-Ni-Ti immersed in ABP presence of 50 ppm of Cholesterol

When Cu-Ni-Ti is immersed in ABP containing 50 ppm Cholesterol the charge transfer resistance R_t increases from 4588 ohmcm^2 to 50094 ohmcm^2 . The C_{dl} value decreased from $1.11 \times 10^{-11} \text{ F/cm}^2$ to $1.0 \times 10^{-10} \text{ F/cm}^2$. The impedance value $\log(Z/\text{ohm})$ decreases from 5.5 to 4.9 These results lead to the conclusion that the protective film is stably formed.

Cu-Ni-Ti immersed in ABP presence of 100 ppm of Cholesterol

When 100 ppm Cholesterol is added the R_t value increases from 4588 to 50094. The impedance value decreases from the 5.5 to 4.9. The C_{dl} value shifted from $1.11 \times 10^{-11} \text{ F/cm}^2$ to $9.7 \times 10^{-11} \text{ F/cm}^2$. Thus the AC impedance study leads to the conclusion that a protective film is formed. When a protective film is formed on the metal surface the face angle value increases. The electron flow through the film from the metal is restricted. It is obtained from phase bode plots the phase angle value decreases in the order of:

$$\text{Cu-Ni-Ti + plasma +100 ppm Cholesterol} > \text{Cu-Ni-Ti + plasma+ 50 ppm Cholesterol} > \text{Cu-Ni-Ti + plasma}$$

The equivalent circuit diagram Cu-Ni-Ti is immersed in various test solution is shown in fig. (6).

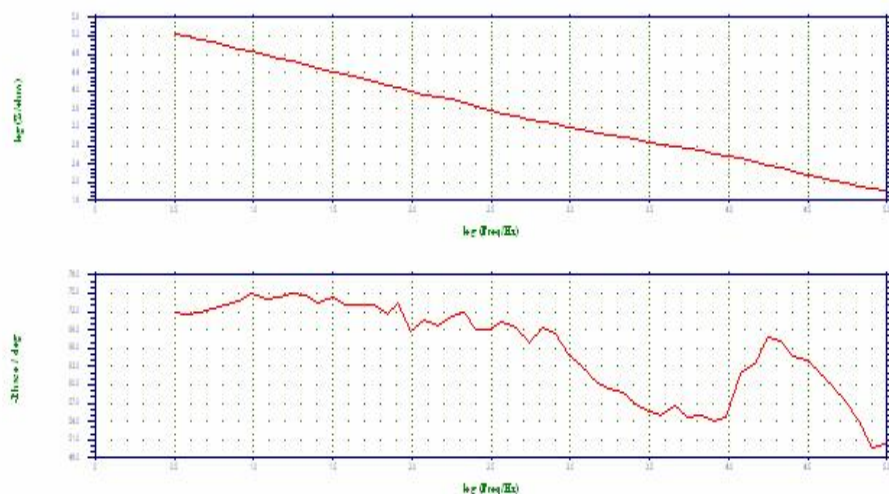


Figure 7 - AC impedance spectra of Cu-Ni-Ti immersed in ABP in absence of Cholesterol (Bode plot).

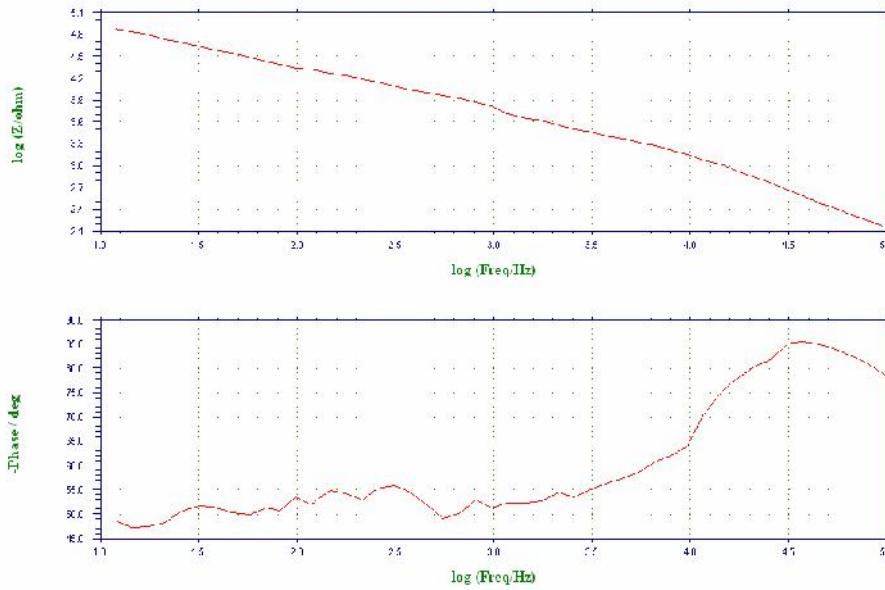


Figure 8 - AC impedance spectra of Cu-Ni-Ti immersed in ABP in presence of 50ppm Cholesterol (Bode plot).

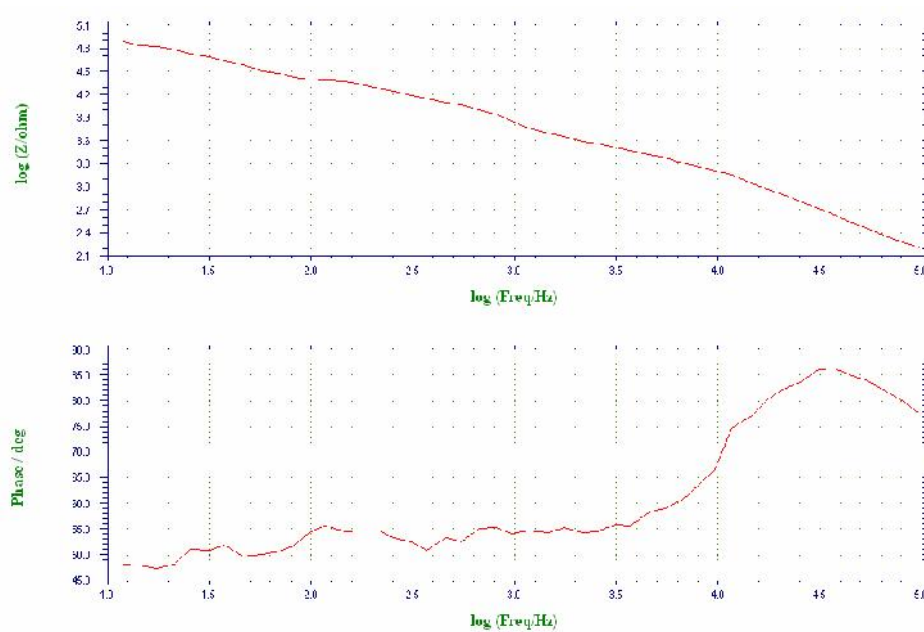


Figure 9 - AC impedance spectra of Cu-Ni-Ti immersed in ABP in presence of 100ppm Cholesterol (Bode plot).

CONCLUSION

The corrosion behavior of Cu-Ni-Ti immersed in ABP in absence and presence of 50 ppm of Cholesterol, 100 ppm of Cholesterol have been studied.

Polarization study leads to the following conclusions:

Cu-Ni-Ti + plasma +100 ppm Cholesterol > Cu-Ni-Ti + plasma +50 ppm Cholesterol > Cu-Ni-Ti + plasma

AC impedance leads to the following conclusions:

Cu-Ni-Ti + plasma +100 ppm Cholesterol > Cu-Ni-Ti + plasma+ 50 ppm Cholesterol > Cu-Ni-Ti + plasma

Acknowledgement

The authors are thankful to the respective management.

REFERENCES

- [1] Ahmed abdelnazeer AS Fouda EA Ashour Inhibition effect of cysteine and glycine towards the corrosion of Cu10Ni alloy in sulphide polluted salt water Electro chemical and impedance study.
- [2] www.wikipedia.com
- [3] A. Krauze, W.Walke, J. Marcinik, Corrosion behaviour of AISI 316L steel inartificial body fluids. Journal of Achievements in materials and manufacturing engineering (volume 31 Dec 2008)
- [4] Rajendran, S., Paulraj, J., Rengan, P., Jeyasundari, J., Manivanna, M. (2009)Corrosion behavior of metals in artificial saliva in present ofspirulinapowder. *Journal of Dentistry and oral hygiene*, 1, 1-8
- [5] Runa, M.J. 2011 Corrosion and tribocorrosion behavior of CoCrMo alloys used as hip joint implant materials under simulated body fluids: Effect of proteins and normal load; *Bioengineering (ENBENG)*, 2011. ENBENG 2011
- [6] S. Rajendran, Ch. Devi, S.John Mary, A. Krishnaveni J., Kanchana, L. Christy, R. Naglakshmi , B. Narayanasamy (2009) Corrosion Behavior Of SS316L In Artificial Saliva In Presence Of Electral; *The Arabian Journal for Science and Engineering, Volume 34, Number 2C*
- [7] American Society for Metals, Metals Handbook, 8thedn, Voll, Metals Part, Ohio, (1968).
- [8] N D. Tomashov and G.P. Chernova, Passivity and Protection of Metals Against Corrosion, Plenum Press, New York (1967).
- [9] M. Stern, J. Electrochem. Soc, 102 (1955), 663.
- [10] Eurocorr 77, The 6 European Congress on Metallic Corrosion (1977), Society of Chemical Industry, London.
- [11] Antony, N., Sherine, H.B., Rajendran, S. (2010) Inhibition and Biocide Actions of Sodium Dodecyl Sulfate-Zn²⁺ System for the Corrosion of Carbon Steel in Chloride Solution; *Portugaliae Electrochimica Acta*, 28(1): 1-14
- [12] Florence, H.R.G., Anthony, N.A., Wilson, S.J., Amalraj, J.A., Rajendran, S. (2005) Influence of cholesterol on the corrosion behavior of copper alloy in presence of artificial blood plasma; *Indian Journal of Chemical Technology*, 12, 472-476
- [13] Gurappa, I. (2002) Characterization of different materials for corrosion resistance under simulated body fluid conditions. *Materials Characterization*, 49(1), 73-79
- [14] Mareci, D., Nemtoi, G.H., Aelenei, N., Bocanu, C. (2005) The Electrochemical Behaviour of Various Non-precious Ni and Co based alloys in Artificial Saliva. *European Cells and Materials*, 10,1
- [15] S. John Mary, S.Rajendran (2011) Corrosion Behavior of Ni-Cr In Artificial Blood Plasma In Presence Of Shelcal-Vitamin D; *Journal of Convergence*, ISSN 0972-6489, 12(1-4),77-84

IZVOD**KOROZIONO PONAŠANJE LEGURE Cu-Ni-Ti U VEŠTA KOJ KRVNOJ PLAZMI U PRISUSTVU HOLESTEROLA**

Koroziono ponašanje Cu-Ni-Ti u vešta koj krvnoj plazmi u odsustvu i prisustvu 50ppm i 100ppm holesterola su prou avani potentiodinami kom polarizacionom metodom i AC impedancom. Efikasnost inhibicije holesterola za koroziju Cu-Ni-Ti se pove ava sa pove anjem koncentracije. Potentiodinami ka polarizaciona metoda pokazuje da je korozija površine metala u velikoj meri smanjena uz prisustvo holesterol. To se može desiti zbog formiranja zaštitnog sloja na metalu u prisustvu holesterola. Studija polarizacije dovodi do inhibicije korozije Cu-Ni-Ti u vešta koj krvnoj plazmi u odsustvu i prisustvu 50 ppm i 100 ppm holesterola i nalazi se u slede em opadaju em nizu:

Cu-Ni-Ti + vešta ka krvna plazma + 100 ppm holesterola > Cu-Ni-Ti + vešta ka krvna plazma + 50 ppm holesterola > Cu-Ni-Ti + vešta ka krvna plzma

Studija AC impedance otkriva da inhibicija korozije Cu-Ni-Ti u vešta koj krvnoj plazmi u odsustvu i prisustvu 50 ppm i 100 ppm holesterola je u slede em opadaju em nizu:

Cu-Ni-Ti + vešta ka krvna plazma + 100 ppm holesterola > Cu-Ni-Ti + vešta ka krvna plazma + 50 ppm holesterola > Cu-Ni-Ti + vešta ka krvna plzma

Ključne reči: korozija, vešta ka krvna plazma, Cu-Ni-Ti, holesterol

Originalni nau ni rad

Primljeno za publikovanje: 13. 03. 2014.

Prihvata eno za publikovanje: 29. 05. 2014.